


Anti-proliferative, pro-apoptotic and anti-invasive effect of EC/EV system in human osteosarcoma

SUPPLEMENTARY FIGURE

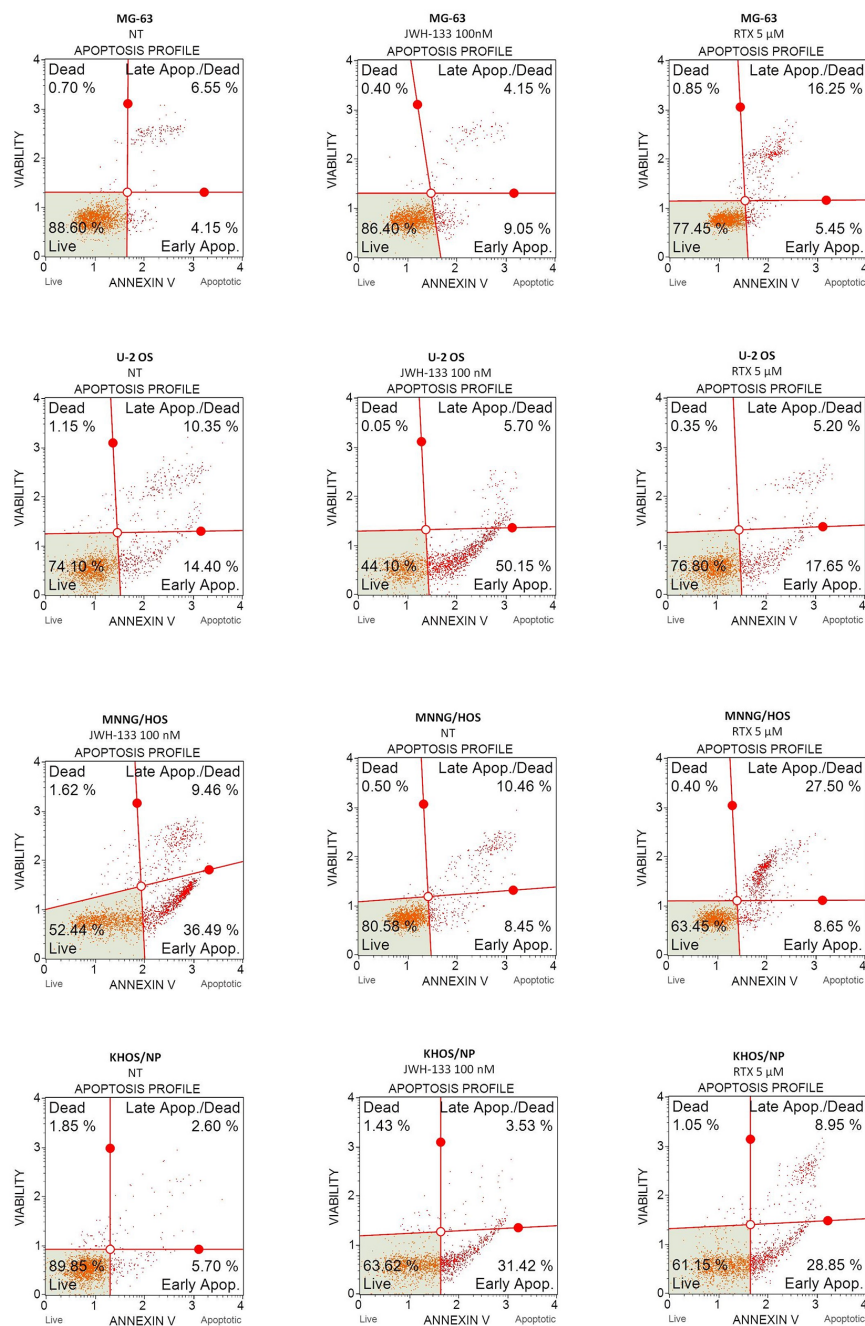

Supplementary Figure 1: Scatter Plots of Apoptosis Assay in JWH-133 and RTX treated OS cell lines. The panels show cytofluorimetric scatter plots representing percentages of apoptosis for MG-63, U-2 OS, MNNG/HOS, Saos-2 and KHOS/NP cell lines. Apoptosis assay was performed using “Cell dead and Annexin V Assay Kit” (Millipore) following the manufacturer’s protocol. The results were obtained with “Muse Count & Viability” software.